



Suresign Vitamin D Rapid Test Cassette (Fingerstick Whole Blood)

Package Insert For Self-testing

OVD-402H English

A rapid test for the semi-quantitative detection of 25-hydroxyvitamin D in human fingerstick Whole Blood.

For self-testing *in vitro* diagnostic use.

【INTENDED USE】

The Vitamin D Rapid Test Cassette is a rapid chromatographic immunoassay for the semi-quantitative detection of 25-hydroxyvitamin D (25 (OH) D) in human fingerstick Whole blood. This assay provides a preliminary diagnostic test result and can be used to screening for Vitamin D deficiency.

【SUMMARY】

Vitamin D refers to a group of fat-soluble secosteroids responsible for increasing intestinal absorption of calcium, iron, magnesium, phosphate and zinc. In humans, the most important compounds in this group are vitamin D3 and vitamin D2.^[1] Vitamin D3 is naturally produced in the human skin through the exposure to ultraviolet light and Vitamin D2 is mainly obtained from foods. Vitamin D is transported to the liver where it is metabolized to 25-hydroxy Vitamin D. In medicine, a 25-hydroxy Vitamin D blood test is used to determine Vitamin D concentration in the body. The blood concentration of 25-hydroxy Vitamin D (including D2 and D3) is considered the best indicator of Vitamin D status. Vitamin D deficiency is now recognized as a global epidemic.^[2] Virtually every cell in our body has Receptors for Vitamin D, meaning that they all require "Sufficient" Level of Vitamin D for adequate functioning. The health risks associated with Vitamin D deficiency are far more severe than previously thought. Vitamin deficiency has been linked to various serious diseases: Osteoporosis, Osteomalacia, Multiple Sclerosis, Cardiovascular Diseases, Pregnancy Complications, Diabetes, Depression, Strokes, Autoimmune Diseases, Flu, Different Cancers, Infectious Diseases, Alzheimer, Obesity and Higher Mortality etc.^[3]

【PRINCIPLE】

The Vitamin D test is an immunoassay based on the principle of competitive binding. During testing, the mixture migrates upward on the membrane chromatographically by capillary action. The membrane is pre-coated with 25 (OH) D antigens on the test line region of the strip. During testing, 25 (OH) D present in the specimen will compete with 25 (OH) D on the test line for limited amount of anti-25 OH Vitamin D antibodies in the conjugate. The higher concentration of 25 (OH) D in the specimen, the lighter would be the T line. The result will be read according to the Color card provided with the kit.

To serve as a procedural control, a colored line will always appear in the control line region indicating that proper volume of specimen has been added and membrane wicking has occurred.

【PRECAUTIONS】

Please read all the information in this package insert before performing the test.

- For self-testing *in vitro* diagnostic use only.
- Do not eat, drink or smoke in the area where the specimens or kits are handled.
- Store in a dry place at 2-30°C (36-86°F), avoiding areas of excess moisture. If the foil packaging is damaged or has been opened, please do not use.
- This test kit is intended to be used as a preliminary test only and repeatedly abnormal results should be discussed with doctor or medical professional.
- Follow the indicated time strictly. Alcohol pad to be used on unbroken skin only.
- Use the test only once. Do not dismantle and touch the test window of the test cassette.
- The kit must not be frozen or used after the expiration date printed on the package.
- Keep out of the reach of children.
- The used test should be discarded according to local regulations.

【STORAGE AND STABILITY】

Store as packaged in the sealed pouch either at room temperature or refrigerated (2-30°C). The test is stable through the expiration date printed on the sealed pouch. The test must remain in the sealed pouch until use. **DO NOT FREEZE.** Do not use after the expiration date.

【MATERIALS】


- | | | | |
|----------------------|---------------------------------|---------------|----------------|
| 1. Test Cassette | 2. Buffer (For single use only) | 3. Lancet | 4. Alcohol Pad |
| 5. Capillary Dropper | 6. Package Insert | 7. Color Card | |

Materials Required But Not Provided

- Timer

【PROCEDURE】

1. Wash your hands with soap and rinse with clear warm water.
2. Bring the pouch to room temperature before opening it. Open the pouch, remove the test cassette and place it on a clean and level surface. Run the test within one hour and best results will be obtained if the test is performed immediately after opening the foil pouch. Remove the dropper, buffer vial, lancet and Alcohol pad, place them close to the test cassette.
3. Carefully pull off and dispose the released cap of the lancet.
4. Use the provided Alcohol pad to clean the fingertip of the middle or ring finger as the puncture site. Allow to air dry.
5. Press the lancet, on the side from where the cap was extracted, the tip retracts automatically and safely after use. Massage the hand without touching the puncture site by massaging the hand towards the fingertip of the middle or ring finger to be punctured.
6. Keeping the hand down massage the end of the finger that was pricked to obtain a blood drop.
7. Without squeezing the capillary dropper bulb, put it in contact with the blood. **The blood migrates into the capillary dropper through the capillarity to the line indicated on the capillary dropper.**
You may massage again your finger to obtain more blood if the blood does not reach the indicated line. Avoid of air bubbles.
8. **Release the blood collected into the Specimen well (S) of the cassette, by squeezing the dropper bulb.**
9. Wait for the blood to be totally dispensed in the well. Unscrew the cap of the buffer bottle and add **2 drops of buffer into the Buffer well (B) of the cassette** and start a timer.
10. Wait for the colored line(s) to appear. **Read results at 10 minutes.** Compare the T line intensity with "Vitamin D Color card" provided with the kit to get the Vitamin D level in your blood. Do not interpret the result after 20 minutes.

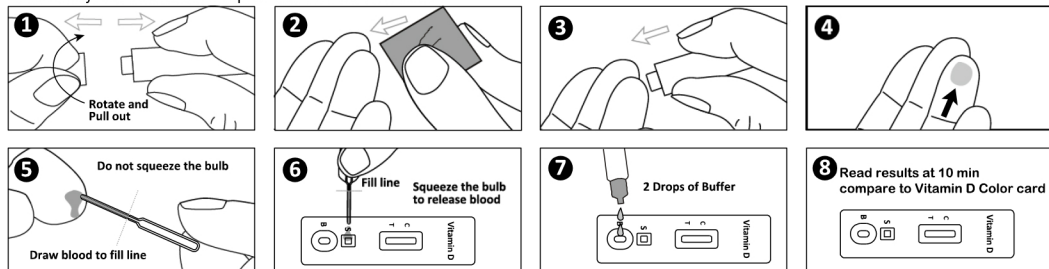

【READING THE RESULTS】

(Please refer to the illustration and compare the T line intensity with "Vitamin D Color card" provided with the kit.)

25-OH Vitamin D Level	Reference Range (ng/mL)	Reference Range (nmol/L)
Deficient	0-10	0-25
Insufficient	10-30	25-75
Sufficient	30-100	75-250



Suresign Vitamin D Rapid Test Cassette (Fingerstick Whole Blood)

Package Insert For Self-testing

OVD-402H English

A rapid test for the semi-quantitative detection of 25-hydroxyvitamin D in human fingerstick Whole Blood.

For self-testing *in vitro* diagnostic use.

【INTENDED USE】

The Vitamin D Rapid Test Cassette is a rapid chromatographic immunoassay for the semi-quantitative detection of 25-hydroxyvitamin D (25 (OH) D) in human fingerstick Whole blood. This assay provides a preliminary diagnostic test result and can be used to screening for Vitamin D deficiency.

【SUMMARY】

Vitamin D refers to a group of fat-soluble secosteroids responsible for increasing intestinal absorption of calcium, iron, magnesium, phosphate and zinc. In humans, the most important compounds in this group are vitamin D3 and vitamin D2.^[1] Vitamin D3 is naturally produced in the human skin through the exposure to ultraviolet light and Vitamin D2 is mainly obtained from foods. Vitamin D is transported to the liver where it is metabolized to 25-hydroxy Vitamin D. In medicine, a 25-hydroxy Vitamin D blood test is used to determine Vitamin D concentration in the body. The blood concentration of 25-hydroxy Vitamin D (including D2 and D3) is considered the best indicator of Vitamin D status. Vitamin D deficiency is now recognized as a global epidemic.^[2] Virtually every cell in our body has Receptors for Vitamin D, meaning that they all require "Sufficient" Level of Vitamin D for adequate functioning. The health risks associated with Vitamin D deficiency are far more severe than previously thought. Vitamin deficiency has been linked to various serious diseases: Osteoporosis, Osteomalacia, Multiple Sclerosis, Cardiovascular Diseases, Pregnancy Complications, Diabetes, Depression, Strokes, Autoimmune Diseases, Flu, Different Cancers, Infectious Diseases, Alzheimer, Obesity and Higher Mortality etc.^[3]

【PRINCIPLE】

The Vitamin D test is an immunoassay based on the principle of competitive binding. During testing, the mixture migrates upward on the membrane chromatographically by capillary action. The membrane is pre-coated with 25 (OH) D antigens on the test line region of the strip. During testing, 25 (OH) D present in the specimen will compete with 25 (OH) D on the test line for limited amount of anti-25 OH Vitamin D antibodies in the conjugate. The higher concentration of 25 (OH) D in the specimen, the lighter would be the T line. The result will be read according to the Color card provided with the kit.

To serve as a procedural control, a colored line will always appear in the control line region indicating that proper volume of specimen has been added and membrane wicking has occurred.

【PRECAUTIONS】

Please read all the information in this package insert before performing the test.

- For self-testing *in vitro* diagnostic use only.
- Do not eat, drink or smoke in the area where the specimens or kits are handled.
- Store in a dry place at 2-30°C (36-86°F), avoiding areas of excess moisture. If the foil packaging is damaged or has been opened, please do not use.
- This test kit is intended to be used as a preliminary test only and repeatedly abnormal results should be discussed with doctor or medical professional.
- Follow the indicated time strictly. Alcohol pad to be used on unbroken skin only.
- Use the test only once. Do not dismantle and touch the test window of the test cassette.
- The kit must not be frozen or used after the expiration date printed on the package.
- Keep out of the reach of children.
- The used test should be discarded according to local regulations.

【STORAGE AND STABILITY】

Store as packaged in the sealed pouch either at room temperature or refrigerated (2-30°C). The test is stable through the expiration date printed on the sealed pouch. The test must remain in the sealed pouch until use. **DO NOT FREEZE.** Do not use after the expiration date.

【MATERIALS】


- | | | | |
|----------------------|---------------------------------|---------------|----------------|
| 1. Test Cassette | 2. Buffer (For single use only) | 3. Lancet | 4. Alcohol Pad |
| 5. Capillary Dropper | 6. Package Insert | 7. Color Card | |

Materials Required But Not Provided

- Timer

【PROCEDURE】



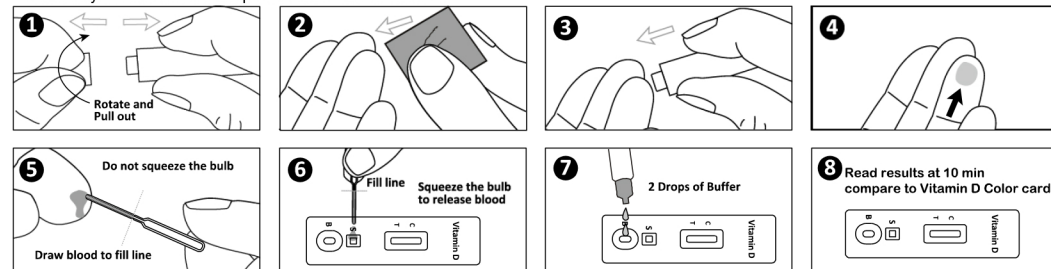


1. Wash your hands with soap and rinse with clear warm water.
2. Bring the pouch to room temperature before opening it. Open the pouch, remove the test cassette and place it on a clean and level surface. Run the test within one hour and best results will be obtained if the test is performed immediately after opening the foil pouch. Remove the dropper, buffer vial, lancet and Alcohol pad, place them close to the test cassette.
3. Carefully pull off and dispose the released cap of the lancet.
4. Use the provided Alcohol pad to clean the fingertip of the middle or ring finger as the puncture site. Allow to air dry.
5. Press the lancet, on the side from where the cap was extracted, the tip retracts automatically and safely after use. Massage the hand without touching the puncture site by massaging the hand towards the fingertip of the middle or ring finger to be punctured.
6. Keeping the hand down massage the end of the finger that was pricked to obtain a blood drop.
7. Without squeezing the capillary dropper bulb, put it in contact with the blood. **The blood migrates into the capillary dropper through the capillarity to the line indicated on the capillary dropper.**
You may massage again your finger to obtain more blood if the blood does not reach the indicated line. Avoid of air bubbles.
8. **Release the blood collected into the Specimen well (S) of the cassette, by squeezing the dropper bulb.**
9. Wait for the blood to be totally dispensed in the well. Unscrew the cap of the buffer bottle and add **2 drops of buffer into the Buffer well (B) of the cassette** and start a timer.
10. Wait for the colored line(s) to appear. **Read results at 10 minutes.** Compare the T line intensity with "Vitamin D Color card" provided with the kit to get the Vitamin D level in your blood. Do not interpret the result after 20 minutes.



【READING THE RESULTS】

(Please refer to the illustration and compare the T line intensity with "Vitamin D Color card" provided with the kit.)

25-OH Vitamin D Level	Reference Range (ng/mL)	Reference Range (nmol/L)
Deficient	0-10	0-25
Insufficient	10-30	25-75
Sufficient	30-100	75-250

 Deficient	Deficient Two distinct colored lines appear. One is in the control region (C) and another should be in the test region (T). The line intensity in the test region (T) is equal to or darker than 10ng/mL line depicted on color card provided with the kit.
 Insufficient	Insufficient Two colored lines appear. One is in the control region (C) and another should be in the test region (T). The line intensity in the test region (T) is darker than the 30 ng/mL line depicted on the color card provided with the kit and lighter than 10 ng/mL line depicted on Color card provided with the kit.
 Sufficient	Sufficient Two colored lines appear, one line should be always in the control region (C) and faint colored line appears in the test region (T). The line intensity in region (T) is equal to or lighter than 30 ng/mL line depicted on Color card.
 Excess	Excess One colored line appears in the control line region (C). No apparent colored line appears in the test line region (T). If the result is excess, it is recommended to consult a physician.
 Invalid	INVALID Control line fails to appear. Insufficient specimen volume or incorrect procedural techniques are the most likely reasons for control line failure. Review the procedure and repeat the test with a new test. If the problem persists, discontinue using the test kit immediately and contact your local distributor.

[LIMITATIONS]

- The Vitamin D Rapid Test Cassette provides only a semi-quantitative analytical result. A secondary analytical method must be used to obtain a confirmed result.
- It is possible that technical or procedural errors, as well as other interfering substances in the whole blood specimen may cause erroneous results.
- As with all diagnostic tests, all results must be considered with other clinical information available to the physician.
- Other clinically available tests are required if questionable results are obtained.

[EXTRA INFORMATIONS]

1. How does the Vitamin D test work?

In medicine, a 25-hydroxy Vitamin D is the main storage form of vitamin D in the body. Therefore, the overall status of vitamin D can be determined by detecting the content of 25-hydroxy Vitamin D. 25-hydroxy Vitamin D level less than 30ng/mL in case of a positive result, indicates Vitamin D **Deficiency or Insufficiency**. Vitamin D supplements can be recommended in these cases.

2. When should the test be used?

The clinical application of 25-hydroxy Vitamin D is mainly for diagnosis, treatment and monitoring of rickets (children), osteomalacia, postmenopausal osteoporosis and renal osteopathy. Vitamin D deficiency is also associated with many other diseases, including cancer, cardiovascular disease, autoimmune diseases, diabetes and depression. Monitor your vitamin D levels to determine whether to take vitamin D supplements. The Vitamin D Rapid Test can be used any time of the day.

3. Can the result be incorrect?

The results are accurate as far as the instructions are carefully carried out. Nevertheless, the result can be incorrect if the Vitamin D Rapid Test cassette gets wet before test performing or if the quantity of blood dispensed in the sample well is not sufficient, or if the number of buffer drops are less than 2 or more than 3. The capillary dropper provided in the box provides a "fill line" indicating the correct volume of blood to collect. Note, due to immunological principles involved, there exists the possibility of false results in rare cases. A consultation with the doctor is always recommended for such tests based on immunological principles.

4. How to interpret the test if the color and the intensity of the lines are different?

Please refer to the illustration and compare the T line intensity with "Vitamin D Color card" provided with the kit.

5. If I read the result after 20 minutes, will the result be reliable?

No. The result should be read at 10 minutes after adding the buffer. The result is unreliable after 20 minutes.

6. What do I have to do if the result is deficient or insufficient?

If the result is deficient or insufficient, it means that the Vitamin D level in is less than 30ng/mL and you should consult a physician, the physician will decide whether additional analysis should be performed.












7. What do I have to do if the result is sufficient?

If the result is sufficient, it means that the Vitamin D level is higher than or equal to 30ng/mL and is within the normal range. A case of Vitamin D toxicity (hypercalcemia), though rare, cannot be excluded based the test result, if symptoms persist, it is recommended to consult a physician.

[BIBLIOGRAPHY]

- Holick MF (March 2006). High prevalence of vitamin D inadequacy and implications for health Mayo Clinic Proceedings. 81 (3): 353–73.
- Eriksen EF, Gierup H (2002). Vitamin D deficiency and aging: implications for general health and osteoporosis. Biogerontology. 3 (1-2): 73–7.
- Grant WB, Holick MF (June 2005). Benefits and requirements of vitamin D for optimal health: a review. Alternative Medicine Review.10 (2): 94–111.


Index of Symbols

	Consult Instructions for Use		Tests per kit		Authorized Representative
	For <i>in vitro</i> diagnostic use only		Use by		Do not reuse
	Store between 2-30°C		Lot Number		Catalog #
	Do not use if package is damaged		Manufacturer		




Hangzhou AllTest Biotech Co., Ltd.
#550, Yinhai Street
Hangzhou Economic & Technological Development Area
Hangzhou - 310018, P. R. China
www.alltests.com.cn

Lancet:



PROMISEMED MEDICAL DEVICES INC.
170-422 RICHARDS STREET,
VANCOUVER BC V6B 2Z4, CANADA

Alcohol Pad:



Jiangsu Sunclean Medical Co.,Ltd
No.11 Fenghuang South Road, Hutang Town, Wujin District
213162 Changzhou City, Jiangsu Province, P.R.China



Ningbo Medsun Medical Co., Ltd.
No. 55 Jinxi Road, Zhenhai 315221 Ningbo
People's Republic of China

Manufactured Under Licence & Distributed By:
CIGA Healthcare Ltd,
Kilcran House, Kildowney Road, Ballymena,
BT44 9EY, Northern Ireland.

REF: OVD-402H
PN: 00690A (SC-202A)
REV: 01/2022

Number: 146625701
Effective date: 2022-04-15



MedNet GmbH
Borkstrasse 10
48163 Muenster
Germany








Lotus NL B.V.
Koningin Julianaplein 10, 1e Verd,
2595AA, The Hague, Netherlands



Medpath GmbH
Mies-van-der-Rohe Strasse 880807
Munich, Germany



Shanghai International Holding Corp. GmbH(Europe)
Eiffelstraße 80
20537 Hamburg
Germany

 Deficient	Deficient Two distinct colored lines appear. One is in the control region (C) and another should be in the test region (T). The line intensity in the test region (T) is equal to or darker than 10ng/mL line depicted on color card provided with the kit.
 Insufficient	Insufficient Two colored lines appear. One is in the control region (C) and another should be in the test region (T). The line intensity in the test region (T) is darker than the 30 ng/mL line depicted on the color card provided with the kit and lighter than 10 ng/mL line depicted on Color card provided with the kit.
 Sufficient	Sufficient Two colored lines appear, one line should be always in the control region (C) and faint colored line appears in the test region (T). The line intensity in region (T) is equal to or lighter than 30 ng/mL line depicted on Color card.
 Excess	Excess One colored line appears in the control line region (C). No apparent colored line appears in the test line region (T). If the result is excess, it is recommended to consult a physician.
 Invalid	INVALID Control line fails to appear. Insufficient specimen volume or incorrect procedural techniques are the most likely reasons for control line failure. Review the procedure and repeat the test with a new test. If the problem persists, discontinue using the test kit immediately and contact your local distributor.

[LIMITATIONS]

- The Vitamin D Rapid Test Cassette provides only a semi-quantitative analytical result. A secondary analytical method must be used to obtain a confirmed result.
- It is possible that technical or procedural errors, as well as other interfering substances in the whole blood specimen may cause erroneous results.
- As with all diagnostic tests, all results must be considered with other clinical information available to the physician.
- Other clinically available tests are required if questionable results are obtained.

[EXTRA INFORMATIONS]

1. How does the Vitamin D test work?

In medicine, a 25-hydroxy Vitamin D is the main storage form of vitamin D in the body. Therefore, the overall status of vitamin D can be determined by detecting the content of 25-hydroxy Vitamin D. 25-hydroxy Vitamin D level less than 30ng/mL in case of a positive result, indicates Vitamin D **Deficiency or Insufficiency**. Vitamin D supplements can be recommended in these cases.

2. When should the test be used?

The clinical application of 25-hydroxy Vitamin D is mainly for diagnosis, treatment and monitoring of rickets (children), osteomalacia, postmenopausal osteoporosis and renal osteopathy. Vitamin D deficiency is also associated with many other diseases, including cancer, cardiovascular disease, autoimmune diseases, diabetes and depression. Monitor your vitamin D levels to determine whether to take vitamin D supplements. The Vitamin D Rapid Test can be used any time of the day.

3. Can the result be incorrect?

The results are accurate as far as the instructions are carefully carried out. Nevertheless, the result can be incorrect if the Vitamin D Rapid Test cassette gets wet before test performing or if the quantity of blood dispensed in the sample well is not sufficient, or if the number of buffer drops are less than 2 or more than 3. The capillary dropper provided in the box provides a "fill line" indicating the correct volume of blood to collect. Note, due to immunological principles involved, there exists the possibility of false results in rare cases. A consultation with the doctor is always recommended for such tests based on immunological principles.

4. How to interpret the test if the color and the intensity of the lines are different?

Please refer to the illustration and compare the T line intensity with "Vitamin D Color card" provided with the kit.

5. If I read the result after 20 minutes, will the result be reliable?

No. The result should be read at 10 minutes after adding the buffer. The result is unreliable after 20 minutes.

6. What do I have to do if the result is deficient or insufficient?

If the result is deficient or insufficient, it means that the Vitamin D level in is less than 30ng/mL and you should consult a physician, the physician will decide whether additional analysis should be performed.












7. What do I have to do if the result is sufficient?

If the result is sufficient, it means that the Vitamin D level is higher than or equal to 30ng/mL and is within the normal range. A case of Vitamin D toxicity (hypercalcemia), though rare, cannot be excluded based the test result, if symptoms persist, it is recommended to consult a physician.

[BIBLIOGRAPHY]

- Holick MF (March 2006). High prevalence of vitamin D inadequacy and implications for health Mayo Clinic Proceedings. 81 (3): 353–73.
- Eriksen EF, Gierup H (2002). Vitamin D deficiency and aging: implications for general health and osteoporosis. Biogerontology. 3 (1-2): 73–7.
- Grant WB, Holick MF (June 2005). Benefits and requirements of vitamin D for optimal health: a review. Alternative Medicine Review.10 (2): 94–111.


Index of Symbols

	Consult Instructions for Use		Tests per kit		Authorized Representative
	For <i>in vitro</i> diagnostic use only		Use by		Do not reuse
	Store between 2-30°C		Lot Number		Catalog #
	Do not use if package is damaged		Manufacturer		




Hangzhou AllTest Biotech Co., Ltd.
#550, Yinhai Street
Hangzhou Economic & Technological Development Area
Hangzhou - 310018, P. R. China
www.alltests.com.cn

Lancet:



PROMISEMED MEDICAL DEVICES INC.
170-422 RICHARDS STREET,
VANCOUVER BC V6B 2Z4, CANADA

Alcohol Pad:



Jiangsu Sunclean Medical Co.,Ltd
No.11 Fenghuang South Road, Hutang Town, Wujin District
213162 Changzhou City, Jiangsu Province, P.R.China



Ningbo Medsun Medical Co., Ltd.
No. 55 Jinxi Road, Zhenhai 315221 Ningbo
People's Republic of China

Manufactured Under Licence & Distributed By:
CIGA Healthcare Ltd,
Kilcran House, Kildowney Road, Ballymena,
BT44 9EY, Northern Ireland.

REF: OVD-402H
PN: 00690A (SC-202A)
REV: 01/2022

Number: 146625701
Effective date: 2022-04-15



MedNet GmbH
Borkstrasse 10
48163 Muenster
Germany



Lotus NL B.V.
Koningin Julianaplein 10, 1e Verd,
2595AA, The Hague, Netherlands



Medpath GmbH
Mies-van-der-Rohe Strasse 880807
Munich, Germany



Shanghai International Holding Corp. GmbH(Europe)
Eiffelstraße 80
20537 Hamburg
Germany